



# IECEX Certificate of Conformity

## INTERNATIONAL ELECTROTECHNICAL COMMISSION IEC Certification System for Explosive Atmospheres

for rules and details of the IECEx Scheme visit [www.iecex.com](http://www.iecex.com)

Certificate No.: **IECEX ULD 18.0013X** Page 1 of 4 Certificate history:  
Status: **Current** Issue No: 2 [Issue 1 \(2019-01-25\)](#)  
[Issue 0 \(2018-09-18\)](#)  
Date of Issue: 2021-11-12  
Applicant: **G.M. International s.r.l**  
Via G. Mameli, 53/55  
20852 Villasanta (MB)  
**Italy**  
Equipment: **Quadruple Repeater Power Supply, D5212Q**  
Optional accessory:  
Type of Protection: **Increased Safety "ec", Intrinsic Safety "ia"**  
Marking: Ex ec [ia Ga] IIC T4 Gc  
[Ex ia Da] IIIC  
[Ex ia Ma] I  
-40 °C ≤ Tamb ≤ +70 °C

Approved for issue on behalf of the IECEx  
Certification Body:

**Erin LaRocco**

Position:

**Staff Engineer**

Signature:  
(for printed version)

*Erin LaRocco*

Date:

2021-11-12

1. This certificate and schedule may only be reproduced in full.
2. This certificate is not transferable and remains the property of the issuing body.
3. The Status and authenticity of this certificate may be verified by visiting [www.iecex.com](http://www.iecex.com) or use of this QR Code.



Certificate issued by:

**UL International DEMKO A/S**  
**Borupvang 5A**  
**DK-2750 Ballerup**  
**Denmark**





# IECEX Certificate of Conformity

Certificate No.: **IECEX ULD 18.0013X**

Page 2 of 4

Date of issue: 2021-11-12

Issue No: 2

Manufacturer: **G.M. International s.r.l**  
Via G. Mameli, 53/55  
20852 Villasanta (MB)  
**Italy**

Additional  
manufacturing  
locations:

This certificate is issued as verification that a sample(s), representative of production, was assessed and tested and found to comply with the IEC Standard list below and that the manufacturer's quality system, relating to the Ex products covered by this certificate, was assessed and found to comply with the IECEX Quality system requirements. This certificate is granted subject to the conditions as set out in IECEX Scheme Rules, IECEX 02 and Operational Documents as amended

## STANDARDS :

The equipment and any acceptable variations to it specified in the schedule of this certificate and the identified documents, was found to comply with the following standards

**IEC 60079-0:2017** Explosive atmospheres - Part 0: Equipment - General requirements  
Edition:7.0

**IEC 60079-11:2011** Explosive atmospheres - Part 11: Equipment protection by intrinsic safety "i"  
Edition:6.0

**IEC 60079-7:2017** Explosive atmospheres - Part 7: Equipment protection by increased safety "e"  
Edition:5.1

This Certificate **does not** indicate compliance with safety and performance requirements other than those expressly included in the Standards listed above.

## TEST & ASSESSMENT REPORTS:

A sample(s) of the equipment listed has successfully met the examination and test requirements as recorded in:

Test Reports:

[DK/ULD/ExTR18.0013/00](#)

[DK/ULD/ExTR18.0013/01](#)

[DK/ULD/ExTR18.0013/02](#)

Quality Assessment Report:

[NO/DNV/QAR07.0005/09](#)



# IECEX Certificate of Conformity

Certificate No.: **IECEX ULD 18.0013X**

Page 3 of 4

Date of issue: 2021-11-12

Issue No: 2

## **EQUIPMENT:**

Equipment and systems covered by this Certificate are as follows:

The D5212Q-xxx module is a galvanic isolator which provides intrinsically safe connections to four field devices (4-20mA transmitters) located in a hazardous area and repeats the transmitter current in the non-hazardous area. 2 channels are also able to accept 4-20 mA current signals from active (powered) transmitter. The DS5212Q is intended for installation in non-hazardous or Zone 2 hazardous locations. It consists of a single PCB assembly in a plastic enclosure suitable for DIN rail mounting or mounting on a termination board (not part of this evaluation). Electrical connections are by means of plug-in terminal blocks or via the termination board. The supply voltage can be optionally provided to the D5212Q by means of the optional Power Bus connector. An optically coupled, open-drain alarm output is also provided. The alarm trip point is settable by the user over the entire input signal range.

**Please see Annex for additional information.**

## **SPECIFIC CONDITIONS OF USE: YES as shown below:**

- For installations in which both the Ci and Li of the Intrinsically Safe apparatus exceeds 1% of the Co and Lo parameters of the Associated Apparatus (excluding the cable), then 50% of Co and Lo parameters are applicable and shall not be exceeded (50 % of the Co and Lo become the limits which must include the cable such that Ci device + Ccable  $\leq$  50 % of Co and Li device + L cable  $\leq$  50 % of Lo). The reduced capacitance of the external circuit (including the cable) shall not exceed 1uF for Groups I, IIA and IIB and 600 nF for Group IIC.
- Isolation in accordance IEC 60079-11 clause 6.3.13 is not provided between separate intrinsically safe circuits. Isolation in accordance with IEC 60079-11 clause 6.3.13 is provided between non-intrinsically safe circuits and intrinsically safe circuits.
- When installed in Zone 2, the unit shall be installed in an enclosure that provides a minimum ingress protection of IP 54 in accordance with IEC 60079-0. The enclosure must have a door or cover accessible only by the use of a tool.
- The equipment shall only be used in an area of at least pollution degree 2, as defined in IEC 60664-1.



# IECEX Certificate of Conformity

Certificate No.: **IECEX ULD 18.0013X**

Page 4 of 4

Date of issue: 2021-11-12

Issue No: 2

## **DETAILS OF CERTIFICATE CHANGES (for issues 1 and above)**

Issue 1: Minor component changes.

Issue 2: Update from IEC 60079-0, Edition 6 to Edition 7 and update from IEC 60079-15, Edition 4, type of protection "nA" to IEC 60079-7, Edition 5.1, type of protection "ec".

## **Annex:**

[Annex to IECEx ULD 18.0013X Issue 2.pdf](#)



# IECEx Certificate of Conformity

Certificate No.: IECEx UL 18.0013X

Issue No.: 2

Page 1 of 3

## TYPE DESIGNATION

D5212Q-xxx, where 'xxx' denotes software or configuration options

## PARAMETERS RELATING TO THE SAFETY

Power Supply: 21.5 to 30 Vdc, 230 mA, 5.2 W

Intrinsically safe specifications:

$U_m$  : 250 Vrms

Terminals		Group IIC	Group IIB or Group III	Group IIA	Group I
13 – 14 (Ch 1) 15 – 16 (Ch 2) 17 – 18 (Ch 3) 19 – 20 (Ch 4)	$U_o$ : 24.1 V $I_o$ : 86 mA $P_o$ : 0.516 W	$C_o$ : 121 nF $L_o$ : 4.85 mH $L_o/R_o$ : 68.9 uH/Ohm	$C_o$ : 917 nF $L_o$ : 19.43 mH $L_o/R_o$ : 275.9 uH/Ohm	$C_o$ : 3307 nF $L_o$ : 38.86 mH $L_o/R_o$ : 551.9 uH/Ohm	$C_o$ : 5197 nF $L_o$ : 63.76 mH $L_o/R_o$ : 905.6 uH/Ohm
21 – 22 (Ch 1) 23 – 24 (Ch 2)	$U_o$ : 1.1 V $I_o$ : 56 mA $P_o$ : 0.016 W	$C_o$ : 99 uF $L_o$ : 11.63 mH $L_o/R_o$ : 2339 uH/Ohm	$C_o$ : 999 uF $L_o$ : 46.54 mH $L_o/R_o$ : 9356.1 uH/Ohm	$C_o$ : 999 uF $L_o$ : 93.09 mH $L_o/R_o$ : 18712.2 uH/Ohm	$C_o$ : 999 uF $L_o$ : 152.73 mH $L_o/R_o$ : 30699.7 uH/Ohm
21 – 22 (Ch 1) 23 – 24 (Ch 2)	$U_i$ : 30 V $I_i$ : 128 mA $C_i$ : 2.1 nF $L_i$ : 0 nH				


## MARKING

Marking has to be readable and indelible; it has to include the following indications:

Certificate No.: IECEx UL 18.0013X

Issue No.: 2

Page 2 of 3

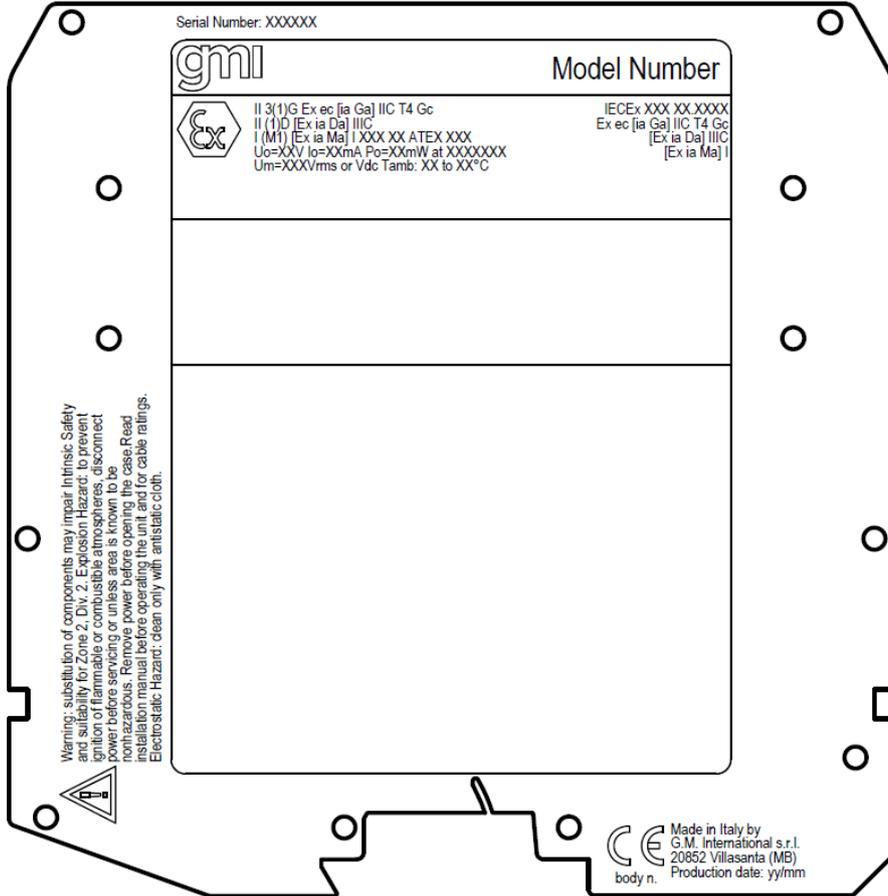

The Label drawing must indicate the following:

Manufacturer: G.M. International 20852 Villasanta Italy (complete address details can be added).

Model Number: D5212Q, D5212Q-xxx.

IECEX Certification: marking indicated in the certificate, certificate number IECEx ULD 18.0013X.

ATEX Certification:  symbol and marking indicated in the certificate, certificate number DEMKO 18 ATEX 2017X.

Electrical Parameters: rated voltage, along with rated current or rated power.

$U_m \leq$  value indicated in the certificate;

$U_o, I_o, P_o \geq$  value indicated in the certificate at terminals 13-14, 15-16, 17-18, 19-20 or at terminals 21-22, 23-24; and

$U_i, I_i \leq$  value indicated in the certificate,  $C_i, L_i \geq$  value indicated in the certificate at terminals 21-22, 23-24.

Ambient Temperature:  $T_{amb} \geq$  lower value to  $\leq$  higher value indicated in the certificate.

Identification Data: Serial Number, Production Date,  logo with the number of notified body for ATEX Quality System certification. Serial number and production date can be encrypted if admitted by the Notified Body responsible for production notification.



# IECEx Certificate of Conformity

---

Certificate No.: IECEx UL 18.0013X

Issue No.: 2

Page 3 of 3

---

## **ROUTINE EXAMINATIONS AND TESTS**

Each piece of equipment shall be subjected to the routine tests for transformers in accordance with clause 11.2 of IEC 60079-11. A test voltage of 1500 Vrms shall be applied between T400A pins 1,2 and T400B pins 1 – 6 for a minimum of 60 s without breakdown resulting in more than 5 mArms flowing. Alternatively a test voltage of 1800 Vrms for a minimum of 1 s may be used.